


```

=====
Acq. Operator   : SYSTEM                               Seq. Line :   40
Sample Operator : SYSTEM
Acq. Instrument : 8860                               Location  :   69 (F)
Injection Date  : 6/14/2024 5:40:17 PM              Inj       :    1
                                                    Inj Volume: 1 µl
Acq. Method     : D:\ChemStation\1\Data\20240614\20240614-280-.M
Last changed    : 6/14/2024 2:27:17 PM by SYSTEM
Analysis Method : D:\ChemStation\1\Data\20240614\20240614-280-.M (
                  Sequence Method)
Last changed    : 6/14/2024 5:52:51 PM by SYSTEM
                  (modified after Loading)
=====
  
```

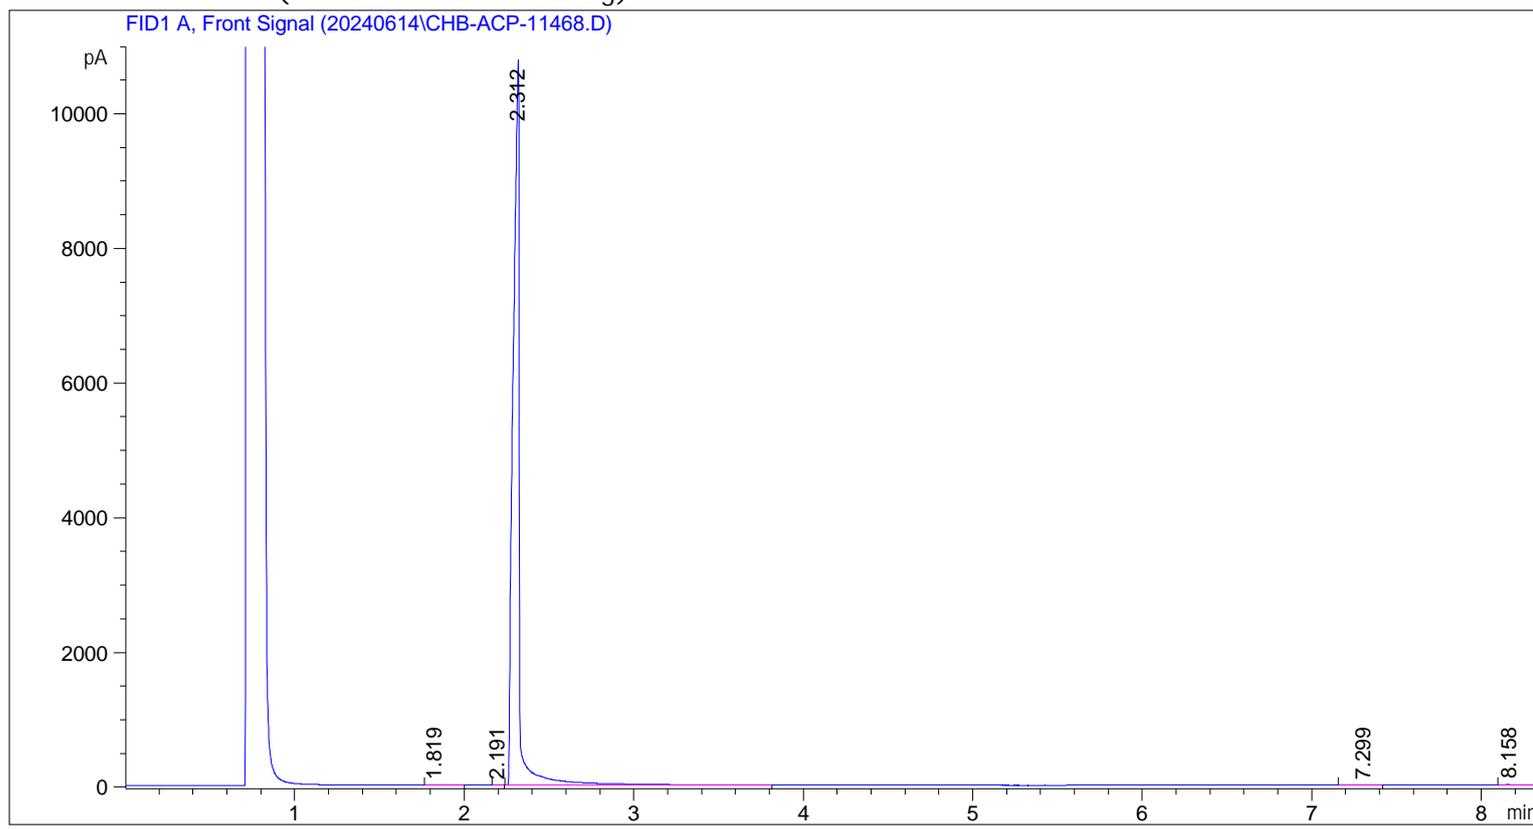

=====
 Area Percent Report
 =====

```

Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Height [pA]	Area %
1	1.819	BB	0.0500	5.25143	1.45736	0.01828
2	2.191	BB	0.0285	2.01008	1.04351	0.00700
3	2.312	BB	0.0502	2.86595e4	9782.99121	99.78711
4	7.299	BB	0.0642	10.13600	2.26381	0.03529
5	8.158	BBA	0.0940	43.74493	6.71128	0.15231

Totals : 2.87206e4 9794.46718

=====
*** End of Report ***